

Report

# Accelerator Beam Centerlines (ABC™) and High Energy Sources (HES) Produced at Varex Imaging Corporation

Andrey Valentinovich Mishin\* 

Industrial Division, HES R&D and ABC Production, Varex Imaging Corporation, Salt Lake City, Nevada, USA

## Abstract

Salt Lake City (Utah) based Varex Imaging Corporation (VREX, NASDAQ), the former imaging components division of Varian Medical Systems, Inc. was spun-off into an independent public company in January 2017. Since the spin-off, Varex has designed, produced, and tested several Accelerator Beam Centerline (ABC) prototypes to meet or exceed the parameters of those previously developed, and some Varex ABC models have been released to production. The primary objective set by Varex was to independently develop Varex's own linear accelerator (Linac) technology that would be a step ahead of current technologies and form the basis of future high energy applications roadmap for Varex; namely, build 3 MeV, 6 MeV, and 9 MeV basic models, in the first place, and eventually, develop advanced products to strengthen Varex's leadership in the field. The fundamental objective has been accomplished and our pilot ABC production line produced 20, 65, and finally, more than twice that much, exceeding 100 units, in consecutive fiscal years of 2022, 2023, and 2024, correspondingly. Our LINAC high-power testing was performed only at our Las Vegas facility, but recently, a test cell at our production facility in Salt Lake City was built in May 2024. A LINAC utilizing 6 MeV ABC represents bulk of Varex units shipped in 2024, the LINAC has been fully tested and released to production in a Diode Electron Gun (DEG) and a Triode Electron Gun (TEG) based versions. A LINAC system Mi6SSM-T is designed based on Mi6SSM product, utilizing TEG and TEG High Voltage (HV) Driver (TEGD). Over 100 new LINAC Systems based on our new ABCs have been shipped to Varex customers. The TEGD is composed in a 19" Mi6SSM rack-mounted assembly, but it can be installed in the LINAC X-ray or Electron Beam Head for designs based on the "legacy" LINATRON® models. In addition, we are developing new linac models. We have designed and tested MicroBeam LINATRON™ with ABC-6-S-M-X-T-SUBMM, delivering less than 500  $\mu\text{m}$  spot size (estimated  $350 \pm 150 \mu\text{m}$ ) and only 12.5% maximum dose rate reduction (700 R/min@1m), compared to a standard ABC-6-S-M-X-T (800 R/min@1m). We have bench-tested a new upgraded M9V accelerator, operating at 9 MeV and delivering substantially higher dose rate (maximum over 5000 R/min@1m) of another contemporary M9 (rated at 3000 R/min@1m). Our new K15V, or V15 (under development) is designed to operate at our common frequency 2998 MHz, and it utilizes a patented hybrid standing and traveling wave design. The first 9 MeV section can be a separate machine (V9), that will deliver very high dose rates, while drastically reducing the produced neutron yields, compared to K-15.

## Keywords

Electron Beam, Linear Accelerators, LINAC, Microwave, Bremsstrahlung, X-Ray, Varex, Imaging, NDT, Security Screening

\*Corresponding author: Andrey.Mishin@vareximaging.com (Andrey Valentinovich Mishin)


**Received:** 12 December 2024; **Accepted:** 22 December 2024; **Published:** 7 January 2025



Copyright: © The Author(s), 2025. Published by Science Publishing Group. This is an **Open Access** article, distributed under the terms of the Creative Commons Attribution 4.0 License (<http://creativecommons.org/licenses/by/4.0/>), which permits unrestricted use, distribution and reproduction in any medium, provided the original work is properly cited.


## 1. Introduction

In January 2017, Varian Medical Systems, Inc. (Varian)<sup>1</sup> completed a spin-off of its imaging components business into a new, stand-alone public company, Varex Imaging Corporation (Varex)<sup>2</sup> (Figure 1).

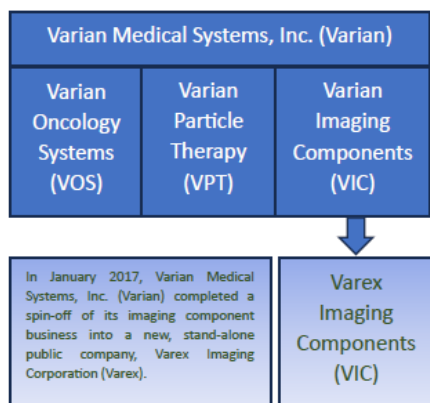

**Figure 1.** Formation of Varex Imaging Corporation (VREX).

Varex is based in Salt Lake City, Utah, and is a leading innovator, developer, and manufacturer of X-ray imaging component solutions. As part of Varex security and industrial business, based in Las Vegas, Nevada, Varex manufactures high-energy linear accelerators (LINACs) (Figure 2). In May 2016, 8 months prior to the spin-off, Varex acquired assets of two small companies:<sup>3</sup> 1) the distribution of Betatrons and detector arrays and 2) development of linear Accelerator Beam Centerlines (ABC). These assets added to Varex's capabilities. Alongside the acquisition of the assets, the Author was hired in a Senior Director role.

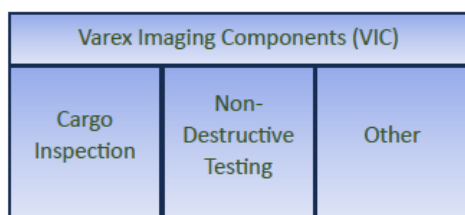


**Figure 2.** Security Screening and Non-Destructive Testing (NDT) Industrial Markets and Products remained with Varex Imaging Corporation after the separation from Varian.

The primary objective set for him was to establish the linac beam centerline production at Varex. Initially, Varex main-

tained a small production line in Fremont, CA, where it continued to produce an X-Band 12 MeV electron beam ABC equipped with a triode electron gun (ABC-12ER-X-E-T), designed by Radmedex LLC (a former company of the Author's) [1, 2] (Figure 3) for an intraoperative radiotherapy system. [3, 4] (Figure 4).

This was necessary to ensure smooth transition of the production, but by the end of 2017, we completely relocated to Varex Headquarters plant in Salt Lake City.

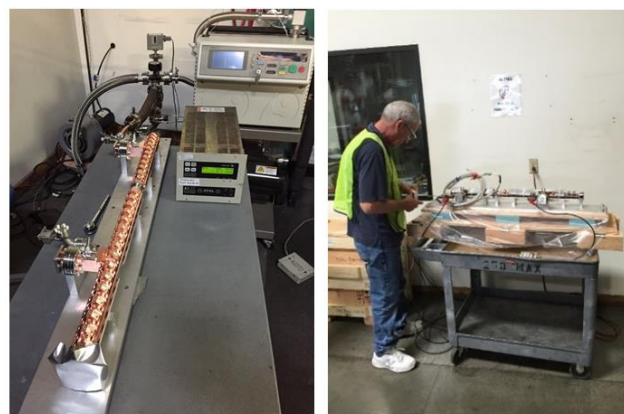

**Figure 3.** 12 MeV electron beam X-Band ABC equipped with a triode electron gun (ABC-12ER-X-E-T).



**Figure 4.** ABC-12ER-X-E-T is utilized on Mobetron System for Intraoperative Radiation Therapy built by Intraop Medical Corporation.

During the past 8 years at Varex Imaging Corporation, we have created a design and production line for Accelerator Beam Centerlines (ABC), built nearly 40 ABC-12ER-X-E-T and now produce our own, independently developed ABCs. In April 2022, the Author was promoted to a position of Vice President in charge of all High Energy Sources R&D and ABC production, combining two groups in Las Vegas (HES or LINAC Systems Development) and Salt Lake City (ABC

<sup>1</sup> <https://www.varian.com/>

<sup>2</sup> <https://www.vareximaging.com/>. The former Imaging Components business of Varian will be referred to as Varex throughout this article.

<sup>3</sup> The companies, Thought One LLC and Radmedex LLC, were dissolved in 2018 after Varex had integrated the relevant assets.

Development and Production). We were able to build an A+ team of Varex professionals, currently 26 people in HES group, who are responsible for many advances and our overall success. We have completed designs of various ABC prototypes, and now we are shipping most of the models and in process of moving all of them to production.

We have reported our progress on ABC and linac systems earlier [5-19]. This manuscript summarizes our work for the past 8 years, the issued patents, and results presented at several professional conferences over the last four years, including the latest IPAC and CAARI in calendar year 2024. During Varex Fiscal Year 2024, which ended 30 September 2024, we produced over 100 ABC, very much meeting goal of the units mix for security, NDT, and other applications. This represents well over 200 percent rate of annual growth during last 3 years (in 2022 and 2023, we produced 20 and 65 ABCs, respectively). We can now claim completion of the original objective, along with many improvements in our ABC performance, which exceeds some features of third-party products. The 3 MeV and 9 MeV production units have been designed and passed Verification and Validation (V&V) process. In addition to these accomplishments, we made some advances in our linac systems, over the last two years since the Author's promotion to a Vice President, R&D in April 2022. The Mi6SSM linac model with a Solid-State Modulator (SSM) (as opposed to "line" modulators) was designed and built in the early days of Varex, and it utilized a diode electron gun with High Voltage (HV) Power Supply (PS), delivered by one of our OEMs. A triode HVPS (TEGD) was also under development at Varex Imaging, which was planned to be a source for a dual switchable energy linac operation, versus an off-the-shelf triode e-gun PS, available in the industry.

Once the Author was put in charge of all HES R&D, we produced a prototype modification of our SSM system Mi6SSM to Mi6SSM-T, combining inherited design of the Triode Electron Gun Driver (TEGD) (alternatively to a Diode E-gun Supply) with the newly produced ABCs with a Triode Electron Gun (TEG), hence expanding the performance range and adding some features combining "High" and "Low" output linacs. We worked on improving TEGD cooling and ruggedness, driving the prototype to a production ready unit. The "T" system is being finalized and moved to production.

The first round of spot reduction effort in our key models resulted in a record small beam spot we obtained in our TEG-based 6 MeV ABC, measured at 0.8 mm [18] (compared to the common 1.5 mm), which may substantially improve image quality. The next round of efforts resulted in building a specialized 6 MeV ABC with a submillimeter spot size, which FWHM we estimate in  $350 \pm 150 \mu\text{m}$ . The next step will be testing the 3 MeV and 9 MeV similar models to the same or less spot size. Finally, our new 15 MeV K-15 system is being redesigned from an operating frequency of 2856 MHz to a common 2998 MHz used for all our other ABCs. This linac design is patent protected [5] and will have a higher average electron beam power (hence, higher dose rate) capability for

high power target testing and operation [16]. It may become our High-Power Platform (HPP) for other systems and applications, including, but not limited to new generation of high-power 9 MeV linac models M9V and an ultra-high-power V9, also operating at 9 MeV and delivering a record high dose rate. The V9 may ultimately be considered a replacement to K-15 in many instances, providing the advantage of much less neutron yield, simpler design, and unprecedented dose rate of the generated Bremsstrahlung.

## 2. Vertical Integration of LINACs using ABC by Varex Imaging

### 2.1. Objective and Conditions

First and foremost, the objective was to secure production of the base models. Directions received from management were as follows:

- 1) Independently develop our own intellectual property and design all the models ourselves,
- 2) maintain a form-factor that would allow using them as replacement in our standard shielding package,
- 3) the new model had to operate using the same or other available power sources and power supplies, such as electron gun high voltage, magnetron input power, etc., and
- 4) The production line capacity to cover full Varex would need to be an estimated 100-200 units/year, considering new product development and future growth.

### 2.2. Challenges and Opportunities

We were facing a complex multifold challenge and had to design prototypes of each linac model, ensure they are working to designated specifications or better with a completely different electron gun operating at 3 times lower voltage, available commercially, which redefined requirements to the linac RF structure - part of the serious challenge. It was clear that under the circumstances, performance of the new ABC would be different, and our job was to develop the new ABCs with specifications as close as possible to our targets with all the other elements of the system remaining the same or similar.

The Triode Electron Gun Driver, or TEGD, later presented another added-on challenge.

It seems that to some degree, all participants fully realized the complexity and scale of this challenge. Ironically, all we had to do in a few years was to design several key models operating the same or better than contemporary technologies and create a production line for these key models "from scratch", catching up with incumbents in the industry that may have spent many decades in perfecting their production, reaching production rates of many hundreds of Beam Centerlines (BCL) per year.

Indeed, Varex wanted reasonably quick completion of the major task. Our expert estimates for the project duration ranged from 5 to 8 years. In the Author's past experience, a full completion and certification of any system prototype would take about 2-5 years, depending on its complexity, and that is only for a single prototype. Now, bringing the product to a complete commercial realization and mass-production could take 8-10 years, and conservatively, in our industry of electron beam linear accelerators for security screening, non-destructive testing, radiation therapy, electron beam processing, it takes 2-5 years for a prototype to become a product ready to mass-produce, and 5-10 years for a production model to fully commercialize and reach top production volume, again, depending on complexity of the product, team maturity, and field of use. Multiple examples can be provided – such as companies and their products, which utilized the linear accelerators the Author participated in developing, such as Mobetron for Intraop, Cyberknife for Accuray, Sentry for AS&E, and a variety of other LINACs [20-40]. A period of 5-8 years seemed reasonable for the multiple developments. Indeed, a staggered schedule helped us to shorten the productization period.

### 2.3. Vision and Strategy

We accepted the challenge in good faith. Our confidence was based on joint extensive experience and a good production base at Varex, hoping to get it to a full success in reasonable period as noted. To “jump-start”, expedite completion, and gain more confidence between the working team and Varex management with every further step at an early phase of the project (during the first couple years), we focused on the most important matters first. The chosen strategy was well-known to the Author; following the proven ways and means, we built working prototypes with a different e-gun, to meet the key specifications, and only then addressing the form-factor and fit. Having designed the linacs independently, and using a different, commercially available 15 kV triode electron gun [41, 42] presented another, separate challenge. This challenge was brilliantly resolved at low cost, and we were able to design to specifications and meet our goals. In addition, we were able to secure three suppliers of the new e-guns.

Running a bit ahead, in 5-6 years from the cold start we realized that our strategy was working, even with many other challenges that have appeared along the way, we continued to gain confidence and got us to full production of the key 6 MeV linac in 2024, in 8 years. We have also completed V&V process for 3 MeV and 9 MeV during the same year, expecting full production for all three models to continue in 2025. In parallel, we have built linacs with both triode and diode electron gun at 3, 6, and 9 MeV, which provides flexibility in the future. Based on internal tests, I believe that our 6 MeV linac with ABC technology demonstrates better performance than other contemporary technologies. We continued implement-

ing a policy of continuous improvements for 3 and 9 MeV linacs, which meets the key specifications at these energy values, but have not yet provided exact match at lower energy. However, we are designing the next generation models, which we believe will meet or exceed previously available specifications in a broad range of electron beam energy. In addition, new initiatives resulting in excellent operational units at various energy values emerged during this journey, and I will be describing them in this monography. Varex's new line of linear accelerators are now called Accelerator Beam Centerlines (ABCs). In the following chapters, we will discuss various ABC models we have put to work at Varex.

### 2.4. 3 MeV Linacs

While it might seem counterintuitive at the first glance, in 2017 we started with designing an X-Band version of a 1.8 MeV LINAC replacement in NX-1 X-Band LINAC, versus more common S-Band frequency band. Based on extensive experience accumulated by the Author in designing and building X-Band linacs for various applications [1-3, 22, 24, 25, 36] and the acquired 12 MeV X-Band linac design from Radmedex LLC, which performance was highly appreciated by the customer [2], it seemed like a great idea – to give Varex management something in a very short timeframe to boost confidence and prove our competence in the subject. The first built ABC is shown in Figure 5.

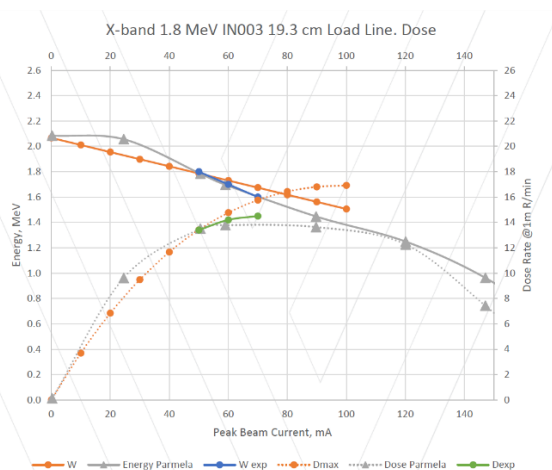


Figure 5. First ABC built and tested at Varex.

#### 2.4.1. ABC-1.8-X-X-T and ABC-3.0-X-X-T

The 1.8 MeV section (Figure 5) was designed for an affordable linac system operating at energy of less than 2 MeV. Regulations associated with lower energy technology substantially broadens the potential geographic market for this linac. Three prototypes have been built, and all demonstrated excellent performance, producing the expected parameters: maximum energy of <2 MeV (contingent on RF power input), with loaded nominal energy of  $1.8 \pm 0.1$  MeV, nominal dose rate of  $13 \pm 2$  Rad/min. The ABC-1.8-X-X is equipped with a triode electron gun and demonstrated a spot size of  $1.0 \pm 0.2$  mm.






**Figure 6.** First ABC Design and Experimental Data using a low power 350 kW magnetron.

The exceptional match between experimental and theoretical data is presented in Figure 6 and in Table 1. Later, this design was used with higher power 800 kW magnetron, it produced a 2.5 MeV beam [5], Figures 7 and 8. In addition, we have decided to test a technique of two separate sections run through a symmetrical 3 dB splitter was described by Victor Vaguine and Eiji Tanabe of Varian [42, 43], also by Getka in [44], producing a dual section LINAC ABC-2.5-X-X-DI with power input through an approximately 3 dB power splitter (Figure 9), otherwise similar in length and performance to the single section ABC (this happened a year later).

The splitter ultimately can replace a circulator, used for isolation of the magnetron from the reflected power from ABC.

**Table 1.** First X-Band Test Results with low-power magnetron.


Parameter	Units	Value
E-Beam Energy		
Design	MeV	1.9
Experiment	MeV	1.8
Dose Rate		
Design	R/min@1m	14.5
Experiment	R/min@1m	12.7
E-Beam Current		
Peak	mA	48
Average	A	37
Magnetron Power		
Peak	kW	359
Average	W	276

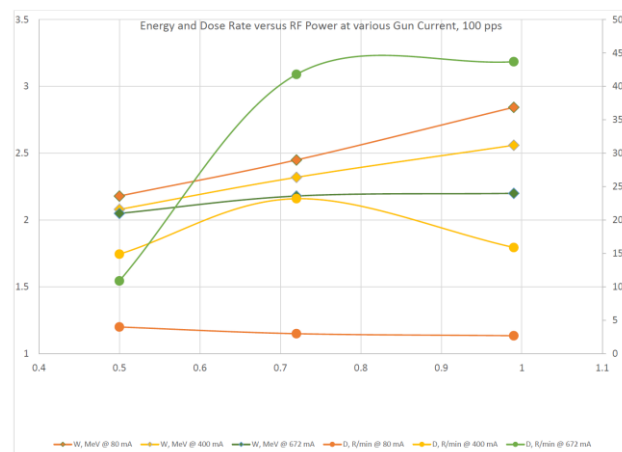

**Figure 7.** ABC-2.5-X-X-T Design and Experimental Data using a higher peak power 800 kW magnetron, 100 PPS.

The symmetrical two-section, dual input through 3 dB coupler design worked very well, and it has a potential for further improvement and cost reduction, or for broad energy and dose regulation, easy low-dose operation, thanks to the triode (gridded) electron gun.

- Setup RF Power to ~0.7MW (Peak)
- Measured Dose and Energy at 400 PPS, 2.2μs Mag I Pulse Width

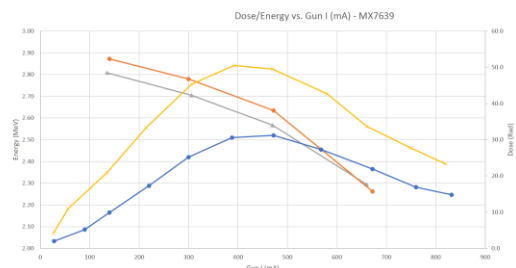

**Figure 8.** ABC-2.5-X-X-T Design and Experimental Data using a higher peak power 800 kW magnetron.



**Figure 9.** ABC-2.5-X-X-DI-T "Dual Input" designed for 2.5 MeV and dose rate up to 50 R/min@1 m from target.

### 2.4.2. ABC-3-S-X Design Strategy and Challenges

Meanwhile, we were gearing up for designing and building the S-Band prototypes and had some choices here. While we still looked at quite a few years ahead until our deadline, the scale and complexity of the task left no illusions and made us pay attention to every detail in building our future strategy, remembering that we had no time to spare. We have analyzed sales data and were facing some choices in priority of the development based on the potential for each linac energy. In addition, challenges with supply of a critical component, the

target, arose, and we urgently needed an alternative solution defined our priorities. As a result, we have focused our efforts on a 3 MeV linac prototype with a different target design. We found that extensive thermal cycling of the targets at a higher pulse repetition frequency reduces life of X-ray targets substantially. Broad regulation of energies and smaller X-ray focal spots are also among the main points of interest from customers. While working on our new guide ABC-3-S-X, we addressed and had initially, at least, a solution for most or all of the problems mentioned above.

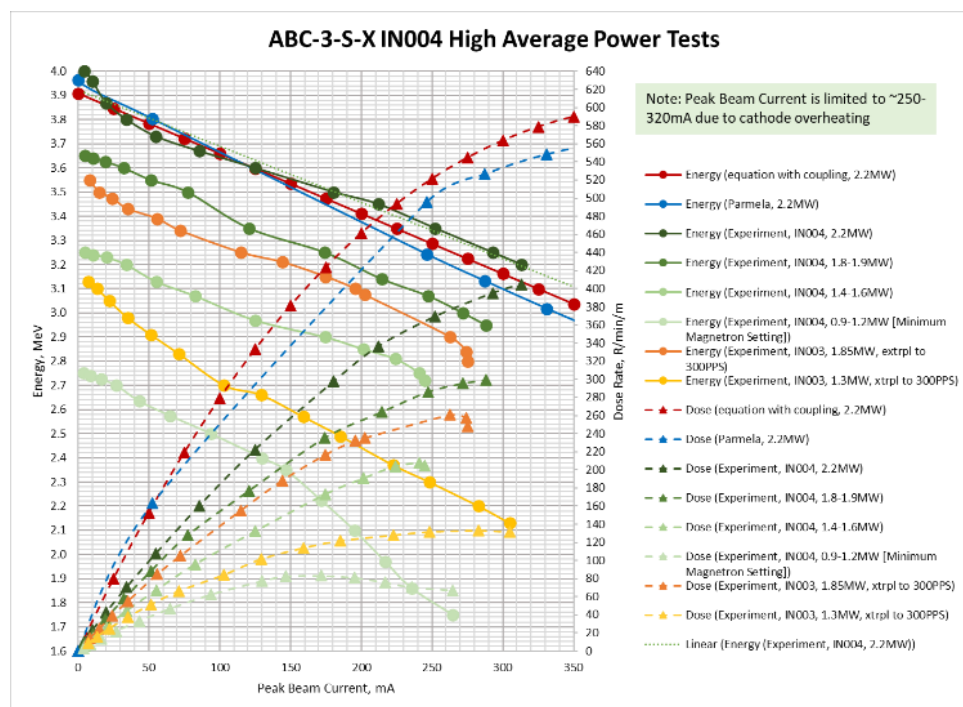


Figure 10. ABC-3-S-O-X-T performance.

A proposed different target design with additional cooling has resulted in extended life. Eventually, the prototype ABC has been run continuously at our customer site, for more than 3000 hours up to date without any issues. In a relatively short beam centerline designed to operate at peak beam currents up to 500 mA where fields are high enough, a so-called beam backstreaming issue is one of the output main limitation factors. By utilizing a powerful beam tracking software Opera, we have been able to improve the electron gun beam optics and, at the same time, restrain beam from striking the electron gun cathode. As a result, we have achieved X-ray dose rate of up to 500 R/min at 1 m from the target. The triode gun helps in a continuous regulation between 2 and 4 MeV while regulating input RF power. The SN004 had produced excellent characteristics, shown in Figure 10, the first time. Not many people might realize that this LINAC is the most difficult one in many aspects – a combination of the high RF power losses per unit length and back streaming bombardment of the cathode due to the LINAC short length present a serious

challenge.

We struggled a bit, trying triode and diode versions, working on a spot size reduction, and went through several design iterations. Finally, in 2018, we produced a prototype version (SN006) that fully met our internal expectations.

### 2.4.3. 1<sup>st</sup> Operational 3 MeV S-Band Prototype Test

This model ABC-3-S-X-D with a diode electron gun marked SN006 has gone through extensive testing at Varex and met the key specification requirements.

Table 2. M3 with our First S-Band ABC-3-S-X-D Test Results.

Parameter	Value
Report Date	3/2/2021
Linac Model	M3

Parameter	Value
Linac Serial Number	3027
Date of New BCL installation	Week of 10/21/2019
Date Testing begun	10/29/2019
Model Number of BCL installed	ABC-3 IN006
Date Focal Spot was measured on	11/7/2019
Focal Spot as measured	1.9 mm
Beam Hours at time of install	2055
Beam hours as of 3/2/2021 5PM EST	3143
Hours run as of 3/2/2021 5PM EST	1088
Dose Rate @ 400 PPS, at 1 m	0.86 Gray/min

\* Notes:

1. Triggered by 1680 Flat Panel Detector Simulator
2. HV Power Supply for Vacion was replaced
3. Thyatron was replaced

Then, it passed life test at a customer [45], the results are presented in Table 2.

While a few further improvements were due, including, but not limited to redesign of the outer shape and changing the form factor to fit the standard shielding package, the results were very positive (see Table 2) and the physics design was complete. This constituted our first substantial step in designing and building the S-Band replacements.

By the end of 2018, we had a group of 7 people and a few ABC models fully designed ready to produce (Figure 11).

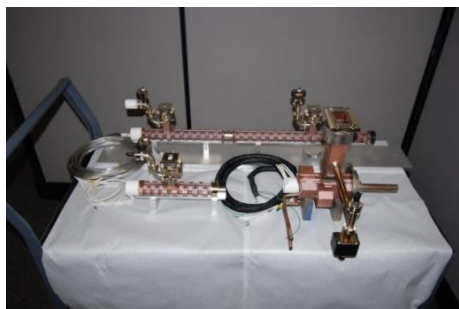


Figure 11. ABC models made available in 2018.

#### 2.4.4. Bringing 3 MeV Design to Production Level

This was our first experience with a diode electron gun, which was a modified version of the standard triode electron gun, and the approach turned out to be a success.

The customer indicated that “there were no issues” in running the unit, confirmed that the parameters met or exceeded the specification, and, most importantly, that the target ran well - no failures observed under same conditions where we experienced multiple failures with the predecessor guides.

Once the 3 MeV prototype met all the requirements, the interim job was completed but it was already 3 years since we started, and while we were working on the 3 MeV prototype, we made a very important strategic decision to postpone further work on the 3 MeV until we master a 6 MeV design. This strategy served us well and was at the very foundation of our overall success. First, the 6 MeV replacement linac represented most of our sales in Security Screening field, and secondly, we had to come up with a common shape to have form-factors for our linacs that met our customers’ requirements.

#### 2.4.5. Closing on ABC-3-S-M-X-T and -D and Further V&V and Certification

Some of the test results on these three units are presented in Tables 3 and 4, with TEG and DEG.

Table 3. M3 initial test with ABC-3-S-M-X-T (SN001-003) E-Gun HV at 8 kV, values averaged for 3 units.

PARAMETER	SN001-SN003	
	3.0 MeV	4.5 MeV
Dose Rate, R/min@1m	172	438
Input RF Power Peak, MW	1.4	2.3
Average, kW	2.6	2.7
Pulse Repetition Frequency, Hz	400	261

Table 4. M3 test with ABC-3-S-M-X-D, RF power varied.

Parameter	Units	SN001 Energy, MeV		SN002 Energy, MeV		SN003 Energy, MeV	
Energy	MeV	1.6	3.1	3.0	4.5	3.2	4.5
Dose Rate	R/min@1m	28	278	130*	298*	298	266*
Spot Size							

Parameter	Units	SN001 Energy, MeV		SN002 Energy, MeV		SN003 Energy, MeV	
Hor.	mm	-	-	1.5**	1.0**	-	1.1**
Vert.	mm	-	-	1.4**	1.3**	-	1.3**
RF Power							
Peak	MW	0.85	1.65	1.3*	1.9*	1.9	1.9*
Aver.	kW	1.5	2.68	2.3	2.65	2.7	2.65
PRF	Hz	400	370	400	315	325	315
E-Gun HV	KV	8.0	11.0	10.4	9.4	14.7	9.4

Skipping this break in our work on 3 MeV line of products and going ahead of myself in our recent Varex history, we will describe closure on 3 MeV “standard” linac replacement in 2024. Three guides have been built and tested, based on the geometry proven in CY2019 - CY2021.

Work on productization of this guide was stalled for a couple years until we mastered the 6 MeV, which, as history showed, was a great decision that allowed us to meet the record system shipment volume in Q4FY23 and in FY24 – over 100 units built and shipped in FY24, when our 6 MeV shipments represented nearly 100% of the revenue.

The three 3 MeV units as originally designed and tested in 2018-2022 were built, successfully passed V&V test, and shipped as part of M3 units to our customers in FY2024. This happened in a matter of several months, versus a couple years it took us to master the first one to work. We were quite happy with this progress.

## 2.5. 6 MeV Linacs

As mentioned earlier, we started design work for the 6 MeV early, and this permitted us to build a few prototypes to get a better feel for the 6 MeV ABC operation. However, we had to work hard - while our built prototypes worked quite well, we had to make several improvements and solve a few puzzles. We worked on this ABC in parallel with building the 3 MeV, and after three iterations of the 6 MeV geometry, ABC-6-S-O-RS-D-X, still in the old “O” style prototype form-factor, met the specifications.

### 2.5.1. First Success on ABC-6-S-O-RS-X-T – Preproduction Certification

The third produced guide ABC-6-S-O-RS-D-X (the Triode version also has been tested, see [Figure 12](#)), still in the old “O” style prototype form-factor, was the first preproduction ABC certification turned out to be successful. Its testing has been completed in early November 2022 (see [Table 5](#)). From the data enclosed in [Table 5](#), one can see that the test results matched the required specification.


**Table 5.** Standard Requirements and Test Results for preproduction 6 MeV ABC-6-S-O-RS-X-T.

Parameter	Units	Value
INPUT DATA		
Magnetron Peak Power		
High	MW	2.3
Low	MW	1.4
E-Gun High Voltage	kV	9.0
E-gun Current		1.4
High	mA	629
Low	mA	668
Duty Cycle		
High		0.0012
Low		0.0009
OUTPUT DATA		
E-Beam Energy		
High, Requirement	MeV	6.0
High, Test	MeV	6.1
Low, Requirement	MeV	3.5
Low, Test	MeV	3.5
Dose Rate		
High, Requirement	R/min@1m	800
High, Test	R/min@1m	818
Low, Requirement	R/min@1m	250
Low, Test	R/min@1m	250

Some results exceeded the expectations, such as focal spot size, which was about two times smaller in diameter, than on



the BCLs.

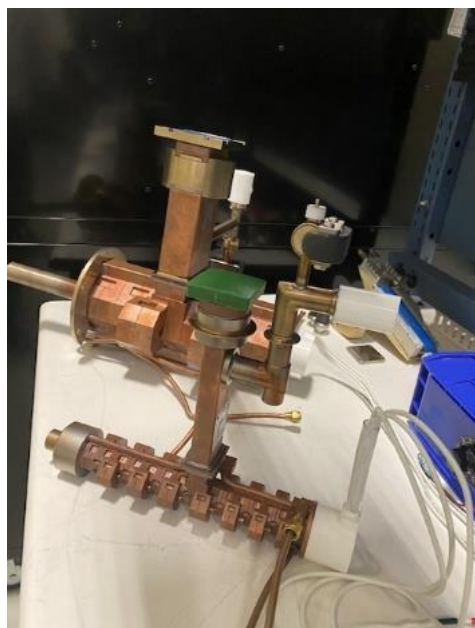


**Figure 12.** ABC-6-S-O-X-T next to ABC-3-X-O-X-T.

### 2.5.2. Production-ready “M” Style 6 MeV

A new cell standard cell design called “M” has been introduced, which had an embedded cooling channel as part of the cell design.


After a few iterations of the 6 MeV geometry, we designed first ABC-6-S-M-RS-D-X, where “M” stands for “Modified” - the new common cell type (and RS - for “Reduced Spot”, as before). The high-power testing of the first prototype was performed in November 2022, right after completion of the first “O” type ABC guide, described earlier.

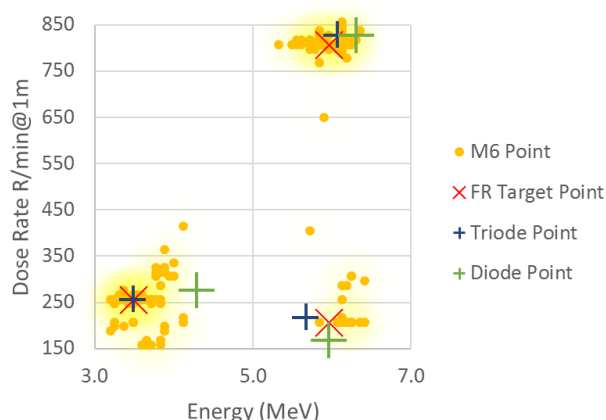

**Figure 13.** Preproduction and M-style ABC-6-S-M in High Dose Operation in comparison with Varian BCL.

several improvements and solve a few puzzles.

The success was obvious, one can see that by simply looking at the charts, shown in Figure 13 and Figure 14 for the High and Low operation, accordingly, both with a triode and diode e-gun – a comparison of the early design to a statistical data collected on third-party guides (marked M6). We had to test both triode and diode e-gun operation of nearly every design, and while our triode design worked right away, we had a few steps to complete with a diode e-gun.

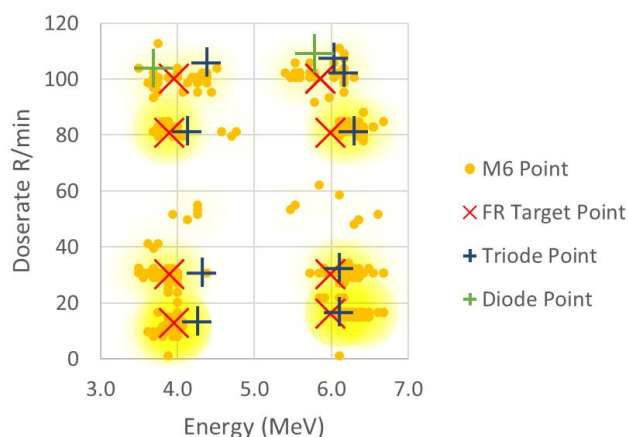

**Figure 14.** Preproduction and M-style ABC-6-S-M in Low Dose Operation in comparison with Varian BCL.




**Figure 15.** ABC-6-S-M-X In order as shown: Final Brazed Assembly (1) Vacuum Assembly ready for vacuum processing (2); Completed, ready to ship ABC-6-S-M-X-D (3).

While the new “M” worked quite well, we had to make

I would mention, once again, that we were attracted to using a triode e-gun, because of ease of driving it to a range of currents at the same voltage, in addition, it permitted working both Low and High modes of operation required by the customer using one single and the same guide, while in a diode configuration, we had to use two different designs. A production unit is shown in Figure 15.

### 2.5.3. Spot Size Reduction in 6 MeV ABCs

In our early designs, we discovered that obtaining a smaller spot requires special attention. The original acceptable beam spots we obtained were on average around FWHM 1.5 mm in diameter, but we substantially improved it in the follow-on units, obtaining spot with FWHM diameter of  $1.0 \pm 0.2$  mm – without any additional external focusing devices [18]. The beam spot shown in Figure 16 has size of 0.9 mm x 0.7 mm FWHM, which perhaps represents a record in the industry for the common commercial linacs with no focusing, and this result (0.8 mm spot) is indeed superior to the third-party guide.

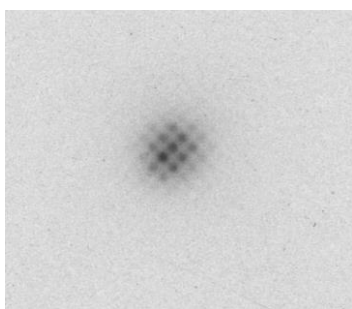

**Figure 16.** X-Ray Spot image taken on a radiographic film using spot camera with ABC-6-S-M-X-D.

We mastered several techniques for beam spot reduction, and eventually, learned how to build ABCs producing the focal spot size of less than 500  $\mu\text{m}$ , establishing a new record in the industry, which is described later in this monography. The latter requires a completely different design of the ABC and a special tuning method that has been developed. The patent is in works and is pending. We called this new line of products MicroBeam LINATRON™ (abbreviated as MBL). In the literature, there are some publications and marketing information stating  $\leq 0.5$  mm spot achieved in linacs [46], but we have not seen any published proof of that, such as spot profiles as measured and/or other similar results. In addition, in many cases an external magnetic focusing system is present, it seems the case in [47-49], in which energy is only 0.95 MeV.

### 2.5.4. Full Production Maturity and Certification of the 6 MeV ABCs

In the following two Quarters (Varex Q2-Q3FY23), we

completed productization of the 6 MeV linacs for Varex. In Q4FY23, we met Varex production demand, followed by full production cycle implemented in FY24, which ended 30 September 2024 with a total of much more than 100 units, most of them 6 MeV ABCs, both diode and triode, delivered. The formal process of moving the ABC design to production has started in FY24 and will be completed in FY25. Meanwhile, we have made small desired remaining improvements and fixed most if not all issues in the ABC design, which were causing any performance flaws in the 6 MeV ABCs. One might appreciate that was done while the rate of ramp-up is truly unprecedented – from 20 units in 2022 to 65 units in 2023 and to more than double the latter number of units in 2024.



**Figure 17.** Varex Corporate Management congratulating HES on opening new Test Cell in SLC.



**Figure 18.** Our HES Las Vegas System Design Group, managed by Rich LaFave (he is waving in the picture).

A test cell was built and commissioned in SLC, in addition to the test cells in Las Vegas, which demonstrated Varex Management firm commitment to further development of the LINAC business.

By now, our team counted 27 people, the Salt Lake City

part of the Team is shown in Figure 17, and Las Vegas part of the Team – in Figure 18.

## 2.6. 9 MeV

We applied the same strategy to the 9 MeV development process, as we did for the 3 MeV. After building the first prototype, which delivered very promising results at the first try, we postponed further development until the 6 MeV has been completed and productized.

### 2.6.1. The First Operational ABC-9-S-O-X-T

The first produced “O”- style guide in 2018-2019 (Figure 19) made all very pleased with its performance. We have built the ABC with an e-beam window to perform accurate measurements of its characteristics. The electron beam energy was measured using multi-plate Faraday Cup, at magnetron peak power of 2.2 MW, E-gun High Voltage of 12 kV, Pulse Length was 5  $\mu$ s, and Pulse Frequency was chosen 50 PPS for this measurement, to keep the average current low and protect the e-beam window from any damage due to extensive heating (Figure 20). We have also produced a few “Beam Trees”, a good visual proof of the linac performance, which have quite an artful appearance and enlightened many of the senior management. Another known name for “Beam Tree” is “Frozen Lightening”.



Figure 19. ABC-9-S-O-X-T being set in a brazing furnace.

The process of forming such a Beam Tree in plastic is quite similar to a natural lightning, hence the name. For those who have never seen or heard of this process, it is as follows. First, in a plastic piece one should make a small notch, usually on the side of the plastic piece near the calculated depth of penetration at given energy.

This will be a discharge point, which is placed on a grounded surface. The accelerated electron beam, coming from the accelerator output window (spread to an appropriate size) is directed at plastic, and the electrons penetrate the plastic, thus forming a space charge, which discharges into the notch once the breakdown voltage limit is reached, leaving the trace, which looks like a lightning.

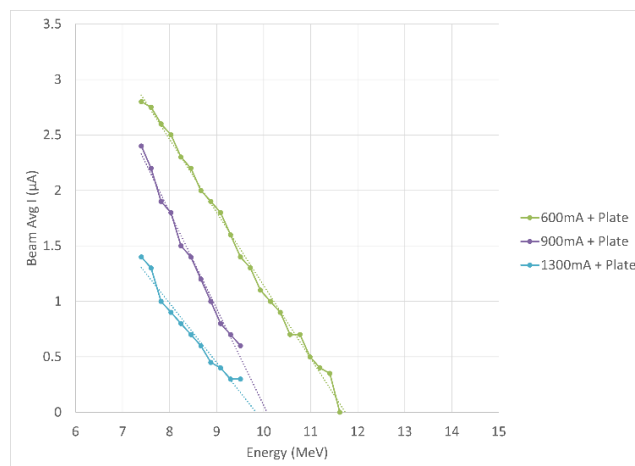


Figure 20. E-Beam Energy Measured for ABC-9-S-O-X-T. SN001 (in 2018) using propagation in Aluminum (Current off plates in FC – tails only), Parameter – E-Gun Peak Current, Penetration is shown in X-Axis and calibrated in MeV.

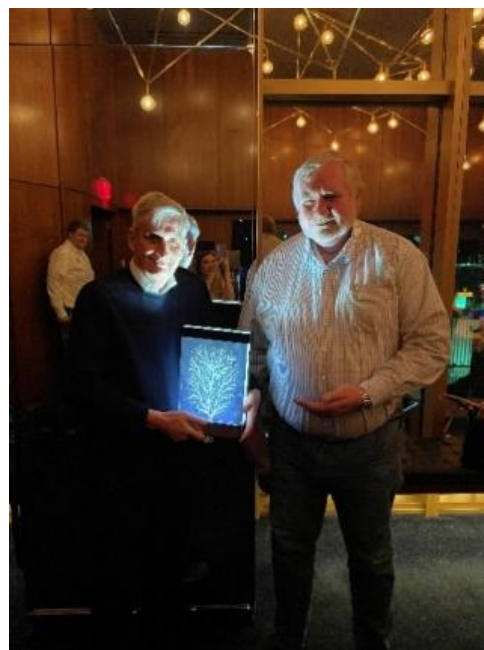


Figure 21. Retirement gift to the Chairman of the Board of Varex Imaging Corporation – a “Beam Tree” created using our first 9 MeV Linac Las Vegas, 9 February 2023.

Some “trial and error” learning is required to produce high-quality “Beam Trees”, but the skilled operators can produce very attractive samples. One of these “Beam Trees”



created using our first 9 MeV has become a gift to our former Chairman of the Board (Figure 21).

### 2.6.2. Preproduction 9 MeV “M” Prototype ABCs Completed in CY2024

While we were closing on productization of the 6 MeV linacs for Varex in Q4FY23, we built and tested a few “M”-style single energy preproduction 9 MeV units. The design was defined earlier by our first model ABC-9-S-O-X-T, which demonstrated good overall performance. Three of the produced units were fully tested with triode and diode electron guns and met the specification requirements. The old design of the LINATRON® M9 used a solenoid, so the guides were built with a RF power input closer to the output end of the LINAC, to ensure a “drop-in” feature present. The required key specification parameters were met. In addition, we started to test modifications, which later brought us to a design functioning well without a solenoid, and in addition, delivering higher dose rate (see paragraph 4 “New Developments at Varex”).

## 3. Completion of Standard 3, 6, and 9 MeV ABCs for M3, M6, M9 and Mi6SSM

With successful completion of full high-power testing of the three 9 MeV ABCs, we declared fulfillment of the original goal of delivering a line of ABCs that could meet customer requirements. Production certification of such ABCs will be fully completed in CY2025. Note that in the light of our preference of building the future models with TEG, we have tested and processed to full production certification of both TEG and DEG versions of such linacs. In the course of building the initial models, we have also reviewed their dual energy performance and possibility of using these ABCs for the “A” dual energy legacy linac models, such as M3A, M6A, and M9A. Needless to say, we were driving to meet the specification requirements for single nominal energy values, and we were using a much lower voltage e-gun, different from the e-gun, used with the third-party guide.

**Table 6.** Comparison of Statistical Energy and Dose Rate data for Varian single energy BCL and Varex ABC designs.

	Varian BCL		Varex ABC	
“3 MeV” Energy, MeV	1.5	3.0	2.0	3.0
Dose Rate, R/min@1m	100	300	120	300
“6 MeV” Energy, MeV	3.5	6.0	3.5	6.0
Dose Rate, R/min@1m	250	800	250	800
“9 MeV” Energy, MeV	6.5	9.5	7.0	9.5

	Varian BCL		Varex ABC	
Dose Rate, R/min@1m	800	3000	600	3000

Therefore, not all the designed single energy ABCs operated the same as the existing legacy units at lower interim energy values with lower injected magnetron RF power, while the maximum specification requirements were identical.

The relatively small difference in dual energy operation of the Varex and legacy single energy models is described in Table 6, above. Due to difference in design, mostly caused by a different e-gun injection voltage, performance of the third-party guide and Varex ABC turns out slightly different, in two out of three cases, but it is close enough for ABC to serve as a substitute. This should not come as a surprise to those skilled in the art.

For the cases when customers are adamant to have closer performance between the two linac generations, we drive to build special units for dual energy operations, especially at 3 MeV and 9 MeV. These special units will be described in the following Chapter 4, targeting better performance than their predecessors, operating in broad energy range and delivering higher dose rate, hence “killing two birds with one stone”.

Our future development strategy is set – we are following our own road maps, unique for Varex, defining our own future and success, helping the customers to adjust and to be more successful together with us. We have already developed exceptional and at times breakthrough designs, and we are hoping that this trend to continue.

## 4. New Developments at Varex

In the past 8 years, we have developed numerous new ABC designs, working on these in parallel with building and replacing the standard units. A few new units are under development, in FY2025, as we discussed, it was an interesting sign that our journey started from building a new X-Band linac, which operated “from scratch”, met the specification delivering an outstanding performance and beam diameter at FWHM of approximately 1 mm, as described in Chapter 2.0. The new X-Band linac flexible design permitted its operation in a broad range of magnetron input power, eventually we built an M3X system based on this ABC. It seems continuing to develop further and produce the X-Band line of products is a low-hanging fruit, but we are quite busy now actively working on S-Band linac developments. We are hoping to eventually get to this X-Band line of products in the next few years, unless we get an inquiry from an interested customer, which might accelerate the X-Band line development.

Below, we present several examples of our new developments, that are currently in process.



We will start with a major success demonstrated in 2018-2019, when we designed a 7 MeV energy-regulated linac, operating in energy range from 3 MeV to 8 MeV, delivering a record dose rate up to 1300 R/min @ 1 m in its maximum [10].


#### 4.1. 3-8 MeV Energy Regulated 7 MeV Linac ABC-7-ER-S-O-X-T

The two versions of ABC-7-S-X have been built – an electron accelerator with a tungsten foil at the output end, and one with an X-ray target. Both have shown outstanding results during high-power testing. Although indirectly measured (with a custom-made Faraday cup in electron case, and via half value level measurement technique in case of X-rays) energy and beam current measurements matched within reasonable margins. ABC-7-S-X has produced up to 1300 R/min maximum dose rate at 6.5 MeV energy. As in the case of ABC-3-S-X, it was measured at 1 m from the target with the 10 x 10 collimator and the ion chamber installed. A triode electron gun helped in establishing smooth energy regulation from 3 to 8 MeV.

Figure 22 illustrates a model of ABC-7-S-X beam center-line and the actual prototype when it was built.

This was major success to have such broad energy range from 3 MeV to 8 MeV, with a record maximum dose rate up to 1300 R/min @ 1 m.


In Figure 23, we present an image of electron beam spot, measured by exposing tape and measuring discoloration of the tape at full width, half maximum (FWHM) of beam distribution. X-ray focal spot has been measured via a grid camera method in which one should take magnification of an X-ray image into account.

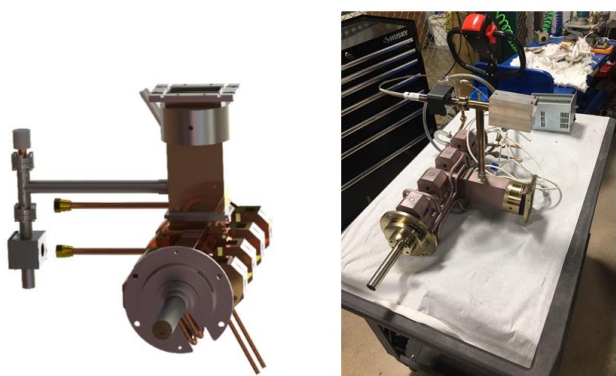

**Figure 22.** ABC-7ER-S-O-X-T SolidWorks model (left) and completed prototype (right), ready for high-power testing.

All the obtained beam spot pictures have been analyzed with Varex developed image evaluation software. For both electron beam spot and X-ray focal spot appeared to be less than 2 mm FWHM at within the whole range of electron beam energy values. At that early phase, we have not yet mastered

the focal spot reduction, as demonstrated later.

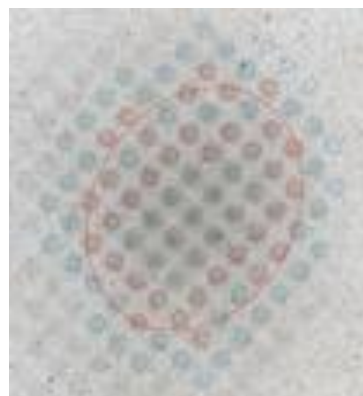


**Figure 23.** An example of ABC-7-S-X X-ray focal spot as seen on a film (scaled).

#### 4.2. New M9V 9 MeV LINAC Substantially Increased Output of its Predecessor M9

We have completed a bench test for a new product, upgraded M9 that we call M9V, featuring our new ABC-9-S-M-T-RL, test setup is shown in Figure 24.

While operating in the similar energy range, it is capable of much higher dose rate, which reaches nearly 5000 R/min@1m at its very maximum, compared to 3000 R/min@1m for its predecessor.

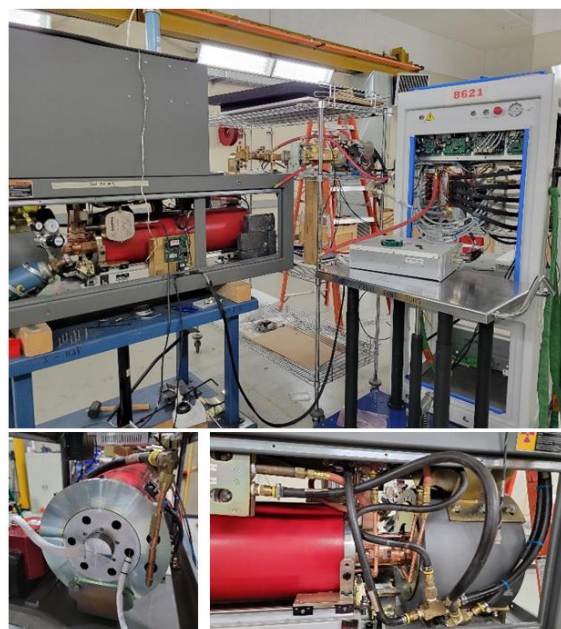

**Figure 24.** M9 LINATRON test assembly with our “drop-in” ABC-9-S-M-X, which demonstrated operation comparable to Varian M9 predecessor at 3000 R/min@1m at its maximum. The upgraded system M9V has been run at a maximum of nearly 5000 R/min@1m.

The complete M9V system will be assembled and fully tested in this FY25 and offered to our customers upon its successful qualification. We are driving for this machine to be based on TEG design for its flexibility and ease of control. Considering that this powerful type of equipment is used for large object inspection, reducing inspection time by 40%-50% will certainly be beneficial to our customers (assuming nominal operating dose rate from 5000 to 6000 R/min@1m). Standby for our updates.

### 4.3. New MicroBeam LINATRON™ Line

This work to produce spots less than 0.5 mm in FWHM diameter has been started at Varex a few years ago “in the background” and has been conducted very thoroughly. This design was one of those dreams the Author had for quite some time, as a few other ideas we are trying and bringing to life at Varex. Another Varex employee challenged the Author to produce the linacs with such small spots.

The proposed approach required some fundamental changes in design of ABC RF structure, as well as a different method of tuning, which has been fully developed, tested, and successfully implemented, patent pending. We believe that the proposed approach permits steady delivery of spots in 100  $\mu\text{m}$  to 500  $\mu\text{m}$  range – and that is without any external focusing systems. Once this range is “tamed”, we might try going below 100  $\mu\text{m}$  to a  $\text{nx}10 \mu\text{m}$  range. The importance of this breakthrough event is very difficult to overestimate, as any commercial linac now can routinely deliver such submillimeter spots – in the fields of non-destructive testing, security screening, in radiation therapy – anywhere one needs crisp imaging and/or tight spots for dose delivering accuracy, while not adding any complex, heavy, and expensive elements, such as external magnets: coils, solenoids, or quadrupoles, at least, until certain point. For example, the first prototype we have built at 6 MeV, resembles the standard ABC-6-S-M and can be used in any field system.


#### 4.3.1. The First “drop-in” 6 MeV SUBMM ABC.

The best developed and productized linac model in house – our ABC-6-S-M-X-T has become a natural candidate for the first try of our new approach. Our design group under Dr. Stanislav Proskin’s supervision made the proposed necessary changes, creating ABC-6-S-M-X-T-SUBMM.

We maintained the form-factor of the guide to make sure we can install it in any standard shielding in our LINAC systems and made the appropriate changes to its RF structure design. Upon design completion, assembling, tuning and standard processing of the guide, we performed a high-power test. The first results were obtained using a “planar camera”, or multilayered plastic/tungsten (or lead) sandwich, where a step between the centers of the tungsten plates or centers of plastic plates equals 0.009” or 0.23 mm, which largely defines resolution of this device, used as is shown in Figure 25.


The obtained images are shown in Figure 26 (left), in

comparison with a standard 1.5 mm spot image (right).

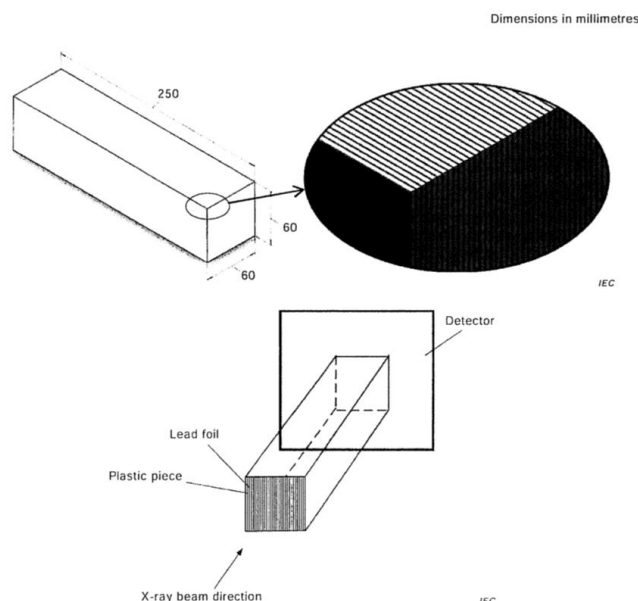

**Figure 25.** Planar Camera or multilayered “Sandwich” first used to make the measurements of Submillimeter beam spots. This technique is well-known and published.


Later, we created overexposed images, shown in Figure 27. Based on the measurements, we concluded that the spot size is approximately  $(350 \pm 150) \mu\text{m}$  at its FWHM diameter. Indeed, resolution of the method was not enough to make more accurate measurement.

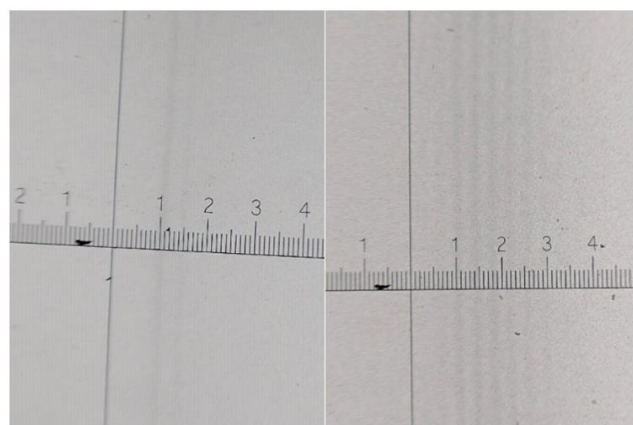

**Figure 26.** Comparison of MicroBeam Spot (left, 2 visible lines, 1 gap) to a Standard 1.5 mm Spot (right, 7 lines, 6 gaps). Visual estimates suggest spot size of 200-300  $\mu\text{m}$  FWHM.


Dr. Martin Hue, who works at Varex and is the lead expert in measuring the spot sizes at Varex Imaging Corporation, and we invited him together with Rich LaFave, head of Las Vegas LINAC System Design group (part of the Author’s

HES group), who also has extensive experience in this field of science, to make the measurements in our test cell in Salt Lake City using Dr. Hue's technique. The results are shown in Figure 28 and Figure 29.

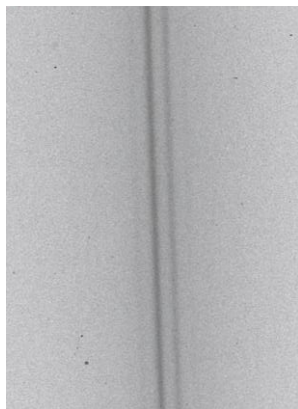

**Figure 27.** Planar Camera overexposed image of the submm spot, 4 lines 3 gaps are visible, which would suggest possible maximum size of the spot of 400-500 $\mu$ m FWHM.

Dr. Hue and Mr. LaFave have concluded that the spot resembles perfect Gaussian distribution, strongly focused (no “tails”), and its measurement resulted in 530x 482  $\mu$ m<sup>2</sup> spot dimensions, followed by double wire test, which suggested D8 image quality with geo magnification 1.91, which is phenomenal, and provides resolution of 184  $\mu$ m horizontally and 171  $\mu$ m vertically. Indeed, we anticipated some measurement error. Operation of the ABC was found to be very steady, although it took about 30 seconds to get fully stabilized at some grid voltages, which we defined later to be a result of some magnetic instabilities combined with specific grid voltage values. We mitigated the problem by using magnetic shield and grid voltages, which ensured steady operation.

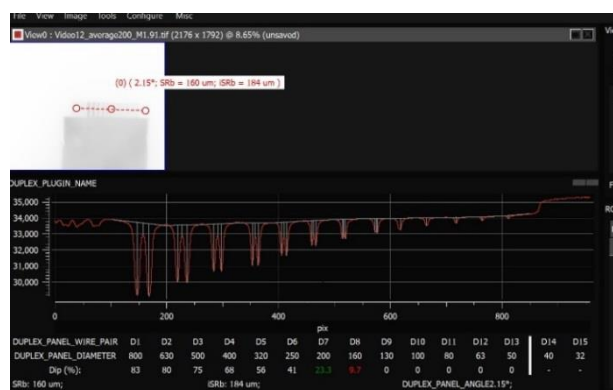


**Figure 28.** ABC-6-S-M-X-T-SUBMM “double wire” test results obtained at the second round of measurements.

One quick imaging attempt using film is shown in Figure


30. Imaging of the watch was performed behind a 1”-inch thick plate. Note that both the front of the watch and the metal strap behind it are visible and present sharp image.

Now that we were convinced the proposed design and method worked, we performed detailed measurements of the E-Beam Energy and produced Dose Rate versus E-beam current and Input Peak RF Power, which is presented in Figure 31.

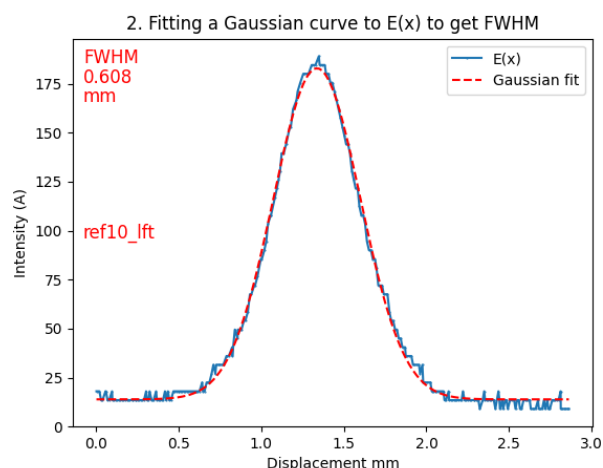


**Figure 29.** One of the ABC-6-S-M-X-T-SUBMM spot scan test results obtained at the second round of measurements.

Currently, we are building a full M6M system prototype and will perform full scale testing of this system, with appropriate imaging tests and looking for ways to further reduce the beam spot. Completion of this work is planned in this FY25. Standby for our updates.

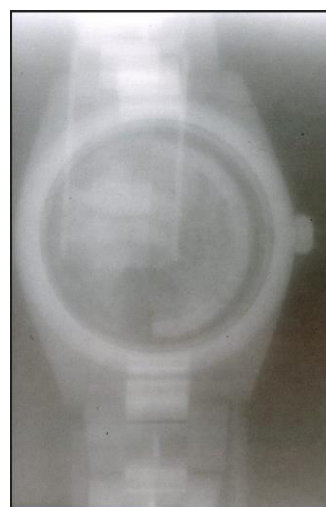

**Figure 30.** A film image of a watch with a metal wrist band behind one-inch-thick steel plate. One can clearly see a thin plate of watch band behind the watch.



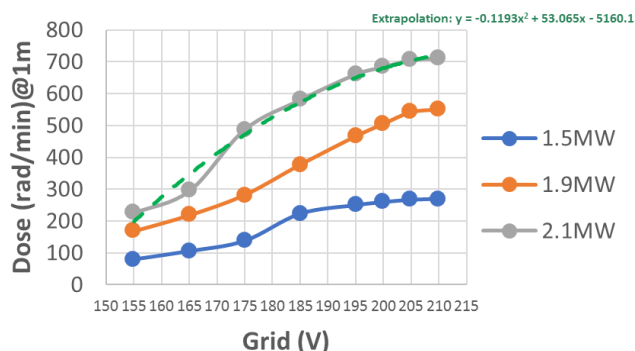

**Figure 31.** Bremsstrahlung Dose Rate produced by 6 MeV MicroBeam LINATRON™ on a tungsten target. Note that at its maximum, it is only 12.5% less than standard specification requirement of 800 R/min@1m, yet the magnetron peak power is 2.1 MW, remains below nominal of 2.3 MW.

#### 4.3.2. The 3 MeV and 9 MeV SUBMM ABC

Currently, we are building 3 MeV and 9 MeV ABC prototypes, using the same technique as we used on the first 6 MeV submillimeter ABC-6-S-M-X-T-SUBMM.

Completion of this work is also planned in this FY25.

Standby for our updates.


#### 4.4. LINAC System Evolution and Mi6SSM

The Figure 32 and Figure 33 provide vision of Mr. Lawrence Miller, our Software Engineer, who happens to be one of the most experienced fellows in control and power electronics in our HES group and leads Control System and System architecture development at Varex. His views are reflecting the development phases for our modulators (Figure 32) and controls (Figure 33).

This vision and the system Mi6SSM (Figure 34), equipped with a Solid-State Modulator (SSM) have been developed before I took charge of the office. Mi6SSM has been designed to operate with third party guides, which use Diode Electron Gun (DEG). For this DEG, a 3<sup>rd</sup> party High Voltage Power Supply (HVPS) is used, which is produced by the same vendor as our SSM. We have designed and built DEG-based ABC-6-S-M-X-D, which is drop-in replacement for the 6 MeV predecessor (while operating at a lower HV of 8-15 kV), as described earlier.



**Figure 32.** Modulator and E-Gun HVPS Evolution.

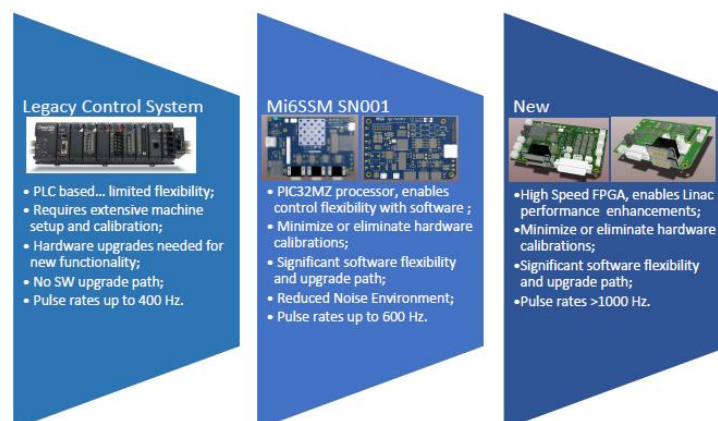

**Figure 33.** System Controls Evolution.



Thus, production of the Mi6SSM has been now fully transitioned to Varex base.

We have inherited the Triode E-Gun (TEG) Driver (TEGD). The first design was completed and tested by Varex prior to me taking the VP job. It worked well in the laboratory environment, but it had to go through several phases of improvements for the field operation, as it was not rugged enough. We are currently completing the third round of such improvements and expect it to be fully production ready in this FY25. In parallel, we are working on several improvements to the original Mi6SSM design.

We intend to drive our TEG design to prevail for the existing and new products, due to better control over the e-beam current in TEG versus DEG.



**Figure 34.** A single block, SSM based Mi6SSM (Tower) LINAC system primarily used for Security Screening. Temperature-Regulated Water Chiller and Operator Console come separately and not shown.


#### 4.5. High Power Platform for 15 MeV V15 – Successor of K-15

As one of the last efforts in this LINAC replacement program, we are considering changing design of our Linatron® K15, the only standard production unit in the world capable of delivering bremsstrahlung at 12000 R/min at 1 meter by striking a stopping target with a high energy Electron Beam (EB) at 15 MeV. We plan on changing the operating frequency from 2856 MHz to 2998 MHz, establishing one common frequency for all our S-Band linear accelerator RF sources. Various designs are being investigated for the new 15 MeV ABC, including but not limited to two collinear standing wave (SW) sections and a Varex patented combination of SW and traveling wave (TW) sections with reverse feeding of RF power [5], see Figure 35. The results of the preliminary analysis have been presented and published at IPAC 2024 [17]. The platform can be used for running guides at various


energy levels from 1 to 20 MeV continuously or selectively changing energy and upgrading the platform to higher average beam power levels. Indeed, operating at high average beam power above 1-2 kW level may require new advanced target development and in the case of e-beam applications, a scan horn will be required for extracting e-beam from vacuum to air.

The new 15 MeV LINAC will be called V15. The 1<sup>st</sup> SW section is based on any of the available standard Varex ABCs, in EB energy range from 1 MeV to 9 MeV. The TW section length will be varied, correspondingly. Overall accelerator length can vary from 1 m to 2 m, depending on the chosen injector and TW section parameters. The RF source power input can vary from 3 MW to 7 MW depending on the optimal length and depending on a chosen RF source.

The first part of this LINAC uses the standing wave section, designed for higher peak and average power and it can be a separate system called V9, shown in Figure 36.

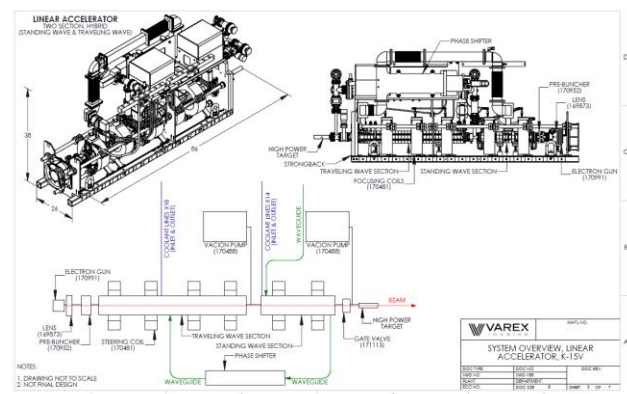

**Figure 35.** Proposed V15 LINAC with hybrid SW and TW structure and reverse feed protected by Varex patent.

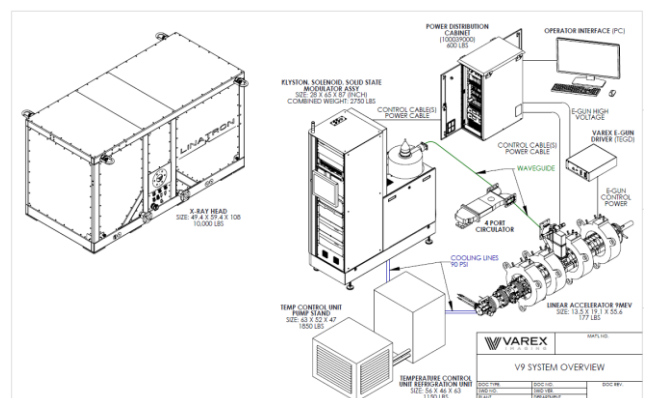

**Figure 36.** First 9 MeV part of V15 - presents a complete V9 linac system, with its own advantages compared to V15.

The Author has presented this concept at CAARI 2024 in Fort Worth, Texas. The V9 machine may have advantages to

V15, such as substantial reduction of the neutron yield and activation of the materials, while maintaining high dose rate.

We intend to use all our advances to produce a small beam spot in V9 system and investigate target behavior at extremely high dose rates of  $\text{nx}10,000 \text{ R/min@1m}$ .

## 5. The Best Results

- 1) As discussed in Paragraph 2.1, the first and foremost objective was to secure production of the base models and build ABC production line, which was met.
- 2) The created new ABC design and production line, which strengthened and broadened capability of Varex Imaging Corporation, which remains a US-based public company on US soil, positioned Varex to become one of the largest domestic LINAC manufacturers, now with unique capability of designing and producing ABC and advanced LINAC systems in-house. It creates a potential for Varex's growth in the existing and several other High Energy Sources markets, beyond security screening and NDT:
  - a) We created our own IP and designed all the LINAC models ourselves,
  - b) We maintained form-factor that would allow using them as replacement in our standard shielding package,
  - c) To the extent possible, the "drop-in" model operation met all specification requirements using the same or other available power sources and power supplies, the exception in the design was the electron gun, available off-the-shelf, that was used in our linacs.
  - d) The production line capacity in 2024 was shown to cover full Varex needs, this number includes new product development.
- 3) We have mastered several novel techniques to substantially improve performance of our ABCs and created or creating prototypes with some outstanding characteristics, as follows:
  - a) Designed and bench tested M9V Linatron, a successor of M9, which can produce much higher dose rate, reaching  $5000 \text{ R/min@1m}$  (versus  $3000 \text{ R/min@1m}$  for M9), the operational prototype is under construction and will be tested in this FY25,
  - b) Upgraded Mi6SSM based on DEG ABC to Mi6SSM-T based on TEG based ABC with increased flexibility,
  - c) Created new unique dual energy designs.
  - d) Designed protection from backstreaming currents for high power LINACs.
  - e) We have created a unique, groundbreaking technique and design, tuning technique to reduce beam spot size, fully tested the first 6 MeV prototype, delivering outstanding results of perfect beam spot of less or equal to  $500 \mu\text{m}$  and now working on a full line of MicroBeam LINATRON<sup>TM</sup> products in a broad EB

energy range, patent pending.

## 6. Discussion

The very nature of this monography is based on replacing the legacy technology by Varex ABCs, and their comparison is presented throughout the manuscript. However, we can summarize the analysis here over larger classes of the devices, such as "Single Energy ABC", firstly.

### 6.1. Single Energy ABC Models

As a starter, here we can reference Table 6 presented earlier in Paragraph 3.0, which provides comparison of the "single" energy linac sections, designed to operate at nominal energy  $W_{\text{nom}}$ , MeV and defining a nominal or maximum dose rate  $P_{\text{nom}}$  R/min@1m at this energy value.

Speaking of the FWHM size, the third-party linacs are usually rated at "less than 2 mm" and practically, they deliver 1.2 mm to 1.8 mm spot sizes, while ABCs are rated from 0.8 mm to 1.2 mm, in most cases; some operate at less than 1.5 mm FWHM size.

All these models are expected to be production certified in FY25.

### 6.2. Dual Energy ABC Models

The Table 6 also shows correlation between the lower energy in the "single energy" guides when input RF power is reduced, and EB current is adjusted accordingly or optimized.

The primary factor is the electron gun design is different between the two, and the operating HV is more than two times lower for ABC, compared to BCL.

The conclusion is that the single energy guides can run in a dual energy mode, but for some units, the lower energy and dose point will be slightly different than in the legacy units.

**Table 7.** Comparison of Statistical Energy and Dose Rate data for Varian dual energy BCL and Varex ABC designs (calculated and rounded data except for measured "7 MeV").

	Varian BCL			Varex ABC	
"3 MeV" Energy, MeV	1.5	3.0	1.0	2.0	3.0
Dose Rate, R/min@1m	100	300	50	150	450
"7 MeV" Energy, MeV	3.5	6.0	4.0	6.5	8.0
Dose Rate, R/min@1m	300	800	350	1300	300
"9 MeV" Energy, MeV	6.5	9.5	4.0	6.0	9.2
Dose Rate, R/min@1m	800	3000	400	1700	3300

To improve operation in broad energy range, Varex created new designs, which we believe will operate better than third-party guides.

For example, our design values for broad energy 1-3 MeV, 3-8 MeV<sup>4</sup>, and 4-9 MeV ABCs are enclosed in a Table 7.

### 6.3. New ABC Models

We are working on improvements of the low-to-medium power linacs and in this manuscript, we described several accomplishments in this area.

We were able to reduce focal spot size in our standard Mi6SSM linac to 0.8 mm, which is one of the best if not the best result in our industry.

We described our new upgraded M9V system, which doubles dose rate compared to its M9 predecessor. This is significant for low power class of such devices.

The most significant accomplishment in terms of its scale certainly was creation of a new design for the MicroBeam LINATRON<sup>TM</sup>, which was an industry scale event and permitted Varex launching off a new unique product line in broad energy range with spot sizes reliably under 500  $\mu\text{m}$ . As discussed earlier, linacs having spots less than 1.0 mm are rather rare and unique: a single design linacs with spot less than 1.0 mm likely used external magnetic focusing system, such as 950 keV X-Band LINAC [46, 47] and/or the Hextron series advertised by GRANPECT did not have any supporting published evidence [45], at least, the Author could not find any. It seems the company removed these “Small Spot Linacs” from their website. At Varex, we developed a new design, which required new tuning method, that can reliably produce small spots of less than 500  $\mu\text{m}$  without any external magnetics and working on further reduction of such focal spot FWHM diameter.

The above results are summarized in Table 8, showing LINACs after various improvements as implemented. Abbreviation MBL6 is used for MicroBeam LINATRON<sup>TM</sup> prototype designed for 6 MeV.

**Table 8.** Comparison of Varian M9 LINAC model and Varex new LINAC models in low-to-medium power range.

OEM	Units	Varian	Varex	Varex	Varex	Varex
Model	N/A	M9	M9V	Mi6SS M	Mi7SS M	MBL 6
Energy	MeV	9.5	9.5	6.0	7.0	6.0
Dose Rate	R/min @1m	3000	5000	800	1000	700
Spot Size	mm	1.2+0.4	1.2+0.4	<1.5	1.0+0.2	<0.5

<sup>4</sup> This 7 MeV model prototype has been built and tested, the 3 MeV and 9 MeV broad energy range prototypes are under construction.

OEM	Units	Varian	Varex	Varex	Varex	Varex
Solenoid	N/A	Yes	No	No	No	No

The MicroBeam LINATRON<sup>TM</sup> Series shown in Table 9 could be compared with key Hextron Small Spot parameters, as advertised in their marketing brochure. However, we do not have information if focusing system is used on such or any data confirming the small spot as advertised. For Varex MBLs, please note that while 6 MeV has been tested, we are still working on 3 MeV and 9 MeV prototypes, and the presented data are design only. While we have high confidence in our success, please wait patiently until the performance can be demonstrated.

We are also working on improvements of the medium-to-high power linacs and described several accomplishments in this area. While there is still a lot of work to be done, we would like to share our goals within our community for their information and planning purposes (Table 10). We welcome the interested customers to send inquiries and discuss their needs early, and we might consider taking the orders sooner rather than later.

Standby for our future updates.

**Table 9.** Varex New MicroBeam LINATRON<sup>TM</sup> Line.

OEM	Units	Varex	Varex	Varex
Model	N/A	MBL3	MBL6	MBL9
Energy	MeV	3 (1-4)	6 (4-7)	9 (6-9)
Dose Rate	R/min@1m	200	700	2000
Spot Size	mm	350+150	350+150	350+150
Solenoid	N/A	No	No	No

**Table 10.** Comparison of Varian K15 LINAC model and Varex new LINAC models in medium-to-high power range.

OEM	Units	Varian	Varex	Varex	Varex
Model	N/A	K15	V15	V9	V9MBL
Energy	MeV	15 (9-20)	15 (2-20)	9 (6-9)	9 (6-9)
Dose Rate	R/min @1m	12000	40000	20000	12000
Spot Size	mm	<2.0	1.2+0.4	1.2+0.4	0.35+0.15
Solenoid	N/A	Yes	Yes	Yes	Yes

## 7. Prospects and Industry Trends

As readers might have noticed, at Varex, we are following the industry trends and current customer demands in the relevant markets of Security Screening, NDT, Electron Beam and X-Ray Processing, such as Sterilization, Pasteurization, Radiation Therapy.

Some requirements are common for all markets, and some are specific to an application.

Reduction of the Focal Spot Size – this requirement benefits mostly Imaging and Radiation Therapy applications. Penumbra prevents creating sharp images in all applications when imaging is required and accurate dose delivery in case of medical applications. For the E-beam and X-ray high power applications, the spot size must be enlarged and, in addition, scanned across the E-beam window or X-ray target in order to reduce power, dissipated per unit area or volume for very high-power beams.

For the Imaging and Radiation Therapy applications, increase of the Bremsstrahlung Dose Rate, produced by the electron beam striking a target is a contradictory requirement to reduction of the focal spot on such target, limited simply by the target temperature, which, in turn, is defined by beam power, dissipated in the target volume, material of the target, its design, etc. Reaching an appropriate balance between the focal spot size and produced dose rate and maximizing the ratio is an art and very difficult to improve for fixed targets. A rotating or simply a "moveable" target for better beam dissipation is an appropriate tool for further improvement.

Improvement of RF-to-Electron Beam efficiency is important across the board for all applications, but it is most important for Processing applications, when power reaches tens and hundreds of kilowatts.

Reduction of size and mass of the irradiators and whole systems is important in any applications, especially those that require any portability and used on gantries and cranes. In addition, mass and size of the machines is directly related to cost reduction, in most cases.

Finally, cost reduction has always been a requirement for the industry to maintain competitiveness. However, the following factors must be considered:

In current markets, cost increase is substantial, for some assemblies, subcomponents, raw materials, cost has nearly doubled.

"We get what we pay for" – usually, considering reasonable approach costs and prices are very similar between producers. As usual, too low and too high costs raise concerns, and defining a reasonable price for current market is a challenge. For a groundbreaking, reliable machine, which has a good life span, premiums are quite appropriate.

OEM qualifications and reputation will define and mitigate many of the unknowns.

The challenge, as always, is that natural increase in cost is ahead of customers' expectations based on the "last year

deliveries", but I guess is a common challenge in any markets.

## 8. Conclusions

This paper summarizes the 8-year history of establishing a completely new for Varex ABC design and production line and describes new designs.

In conclusion, the Author would like to emphasize, once again, that we have improved and strengthened Varex LINAC production by establishing ABC design and production line, also strengthening Varex's leadership position in linac design and production.

We have developed new ABCs at Varex Imaging that meet or exceed the performance of some third-party LINACs. While Varex remains an undisputed leader in production of the tubes, panels, and other imaging technology, it is our intent to continue our improvement and growth, support our customers and become a leader in the industry of High Energy Sources – Linear Accelerators for a variety of applications, which include, but not limited to Security Screening, Non-Destructive Testing, Electron and X-Ray Radiation processing – sterilization, pasteurization, Radiation Therapy.

We take this duty very seriously, so please do contact us with your needs and we will work with you to tailor solutions to your requirements.

In addition, we request the scientific and engineering community: please do contact us with any feedback and questions.

We are hoping that our customers and interested parties will follow our publications at many professional conferences – we are hoping to gain your interest in our existing and new products.

## Abbreviations

HES	High Energy Sources
BCL	Beam Centerline (used for Legacy Linacs)
SW	Standing Wave
TW	Traveling Wave
ABC	Accelerator Beam Centerline (Varex Product)
LINAC	Linear Accelerator
HV	High Voltage
HVPS	High Voltage Power Supply
DEG	Diode Electron Gun
TEG	Triode (Gridded) Electron Gun
TEGD	Triode (Gridded) Electron Gun Driver
FWHM	Full Width at Half Maximum
EB	Electron Beam
IP	Intellectual Property
MBL	MicroBeam LINATRON™



## Acknowledgments

The Author apologizes in advance for this long “Thank-you” list, which he tried to make shorter, unsuccessfully. In fact, it should be much longer, and the Author is sorry if he has missed some of the names here, but rest assured that all help, contributions, good will, and friendship is remembered and cherished.

As always, the Author would like to honor memory of his late mentors, colleagues, and friends, also, honor those who are still living: all professors and teachers at the University (MEPhI), especially, Dr. Igor Shchedrin, his supervisor and mentor in the engineering profession, graduate work, and later, Ph.D. Thesis; Professor Nikolay Sobenin, who was scientific advisor to Dr. Shchedrin, thus, Author’s “scientific grandfather”. It was a pleasure to host Prof. and Mrs. Sobenin as guests at the Author’s house, when they visited the USA.

To Mr. Russell Schonberg – a legend entrepreneur, who left brothers Varian and founded his own company Schonberg Radiation (later changed to Research) Corporation (SRC), who has become Father of the X-Band linacs in the USA, and to all his family, all SRC employees, and employees of the successor – AS&E High Energy Systems Division, who truly changed Author’s life following a job offer from Russ in 1992 and his mentorship ever since, to Bob and Marianne Hamm, also the legends in the industry, who introduced the Author to Russ in 1992, Mr. Hank Deruyter, Dr. Ted Roumbanis, Dr. Roger Miller, Dr. James Potter – well-known stars and classics in the world of accelerators, and many others - all receive the Author’s great appreciation. He will always treasure their invaluable contributions and mentorship and devotes all his technical achievements to them. More great “old timers”, many have become my mentors and friends, Professor Richard Lanza, Dr. Eiji Tanabe, Mr. Greg Cody (retired), Dr. Alan Todd, and many others. In the corporate world, the Author also had several business mentors, some he reported to after we sold Schonberg Research to AS&E. Many thanks to Mr. Ralph Foose, who played a big role in Author’s professional growth and for Ralph’s kind letter of recommendation to the United States Government. Ralph’s guidance in Operations and other business matters, also, his shared general wisdom while the Author served as a General Manager of HES Division at AS&E and later, after relocation to Massachusetts, were invaluable. Working side by side with Ralph, sometimes for 18 hours straight, the two have made many accomplishments. Ted Owens, CFO at AS&E has greatly grown Author’s skills in business and finance, he also consulted for his LLCs. Mr. Ralph Sheridan, CEO, all his entire staff, AS&E Board members shared their wisdom, which served the Author for years, in many ways. A sincere “thank you” to Mr. Anthony Fabiano, CEO of AS&E, successor of Mr. Ralph Sheridan, the Author keeps great memories about working under his guidance and knowing him as a person. Being part of a group that created a miracle of growing AS&E stock nearly 10 times was a trill and a great learning experience. Mr. Ken Breur, SVP of AS&E,

who continued training the Author in operations, and later, a minority shareholder and partner in his LLC, his wife Mrs. Eileen Breur have become good friends – a big “Thank you!” to both. Many thanks to Varex Senior Management and personally to Mr. Sunny Sanyal, CEO for trusting the Author with this latest important assignment described in this manuscript. The Author extends gratitude for direction and educational experience to all supervisors during his career at Varex – Dr. Robert Drubka (who was the initiator and the driver behind acquisition of assets of Author’s LLCs by Varian), Mr. Mark Jonaitis, Mr. Carl LaCasce, Mr. Steven DeVita, Mr. Jesse Merkley, and all at Varex who supported and guided him throughout the years of employment. Finally, many thanks to the Author’s brilliant team at Varex: Ms. Yvette Toombes, Dr. Stanislav (Stas) Proskin (also Dr. Shchedrin’s student like the Author), who become the best trainee, employee, and life-time supporter. The Author was happy to mentor Stas for over 10 years. Mr. Rich LaFave, who has been a good friend and advisor to the Author at Varian and Varex from day one, Mr. Loren Young, an outstanding Production Manager who has helped the Author in growing Varex ABC production from the ground up to over 100 units/year in 2024, and Mr. Aren Anderton, High Power Test Manager, who is another rising star in the group, responsible for many breakthroughs under Author’s guidance. It is a result of the team hard work that gave birth to so many outstanding accomplishments. The Author thanks all colleagues across the industry, customers, and vendors, many have become personal friends, Mr. Mikael Lindholm, Mr. Sergey Novikov, Dr. Aleksandr Sidorov, others of Indicom, Dr. Michael Shtein, Mr. Victor Shcherbinin, others of Foton, Mr. Roman Gubert, Mr. Vijay Alreja, Mr. Al Luna, and many, many others who were so dedicated to the task and supported the Author in his journey. A warmest “Thank You” to Author’s wife Aleksandra (Sasha), who he married in 2016, after his divorce with Galina in 2015. Since day one after their meeting, Sasha has become a dear friend and supporter. Also, the Author sends a big and warm “Thank You” to all his children, especially to his son Andrew and Andrew’s wife Bri; also, to Vasilii, Sasha’s son – the Author has gained two more wonderful children - Vasilii and Bri have become another son and daughter, the Author thanks them for their wisdom, kind hearts, support, care, and love they provide to him and Sasha. Author’s gratitude to his extended family, those who passed and those are living, dear late parents, Valentin and Larisa Mishin, late grandma Olga and others, to all relatives who helped in his life and professional journey and especially, Author’s older sister Liudmila. Thanks to ex-wife Galina for 32 years together and for the two children they had. Lastly, the Author would like to thank his closest and dearest friends: Aleksandr Yudin, Sergey Patronov, and now late Mikhail Vinokurov for their everlasting friendship and support since High School.

“Thank you, all! Please forgive for everything and anything that you think was not right. May The Lord bless you all and forgive you all!”

## Author Contributions

Andrey Valentinovich Mishin is the sole author. The author read and approved the final manuscript.

## Funding

All work carried out in 2016-2024 has been financed by Varex Imaging Corporation, no Government funding has been used.

## Data Availability Statement

The data supporting the outcome of this research work has been reported in this manuscript and provided references.

## Conflicts of Interest

The author declares no conflicts of interest.

## References

- [1] A. V. Mishin, H. DeRuyter, T. Roumbanis, and R. G. Schonberg, "Intraoperative X-Band Accelerator Microwave Structure Design", in *Proc. EPAC'94*, London, UK, Jun-Jul. 1994, p. 2185-2188.
- [2] A. V. Mishin, S. S. Proskin, New Generation X-Band LINACS for Industrial and Medical Applications, Proceedings of IPAC2013, Shanghai, China, 2013.
- [3] R. G. Schonberg, A. V. Mishin, New Medical Linacs, Proceedings of 14th CAARI-96 Conference, Denton, Texas, 1996. <https://doi.org/10.1063/1.52437>
- [4] Intraop Medical Corporation HQ, 150 Almaden Blvd., Suite 150, San Jose, CA 95113, <https://www.intraop.com>
- [5] A. V. Mishin, Hybrid Standing Wave/Traveling Linear Accelerators, Patent Application Serial No. 15/456,057, Docket No. 13-033-US-C1, Filed March 10, 2017, Patent date July 3, 2018, US Patent 10,015,874.
- [6] A. V. Mishin, Transmission Target for High Power Electron Beam, Patent Application Serial No. 18/985,677, Docket No. 2017-175-US1, Filed May 21, 2018, Patent date May 18, 2021, US Patent 11,011,341.
- [7] A. V. Mishin, Multiple Head Linac System, Patent Application Serial No. 62/740,529, Docket No. 2018-033-US1, Filed October 3, 2018, US Patent No. 11,089,670 B2 granted 10 August 2021.
- [8] A. V. Mishin, "New Accelerator Beam Centerline (ABC) Production Line at Varex Imaging Corporation", in *Proc. IPAC'21*, Campinas, Brazil, May 2021, pp. 1087-1089. <https://doi.org/10.18429/JACoW-IPAC2021-MOPAB349>
- [9] Andrey V. Mishin, Matthew Denney, Devon Fischer, Stanislav Proskin, Kade Brown, Nathan Paul Hanson, John Stammetti, Portable 2.5 MeV X-Band Linear Accelerator Structure, IPAC2021, Proceedings of IPAC2021.
- [10] S. Proskin, D. Fischer, and A. V. Mishin, "New 3 MeV and 7 MeV Accelerators for Cargo Screening and NDT", in *Proc. IPAC'21*, Campinas, Brazil, May 2021, pp. 2491-2493. <https://doi.org/10.18429/JACoW-IPAC2021-TUPAB412>
- [11] A. V. Mishin et al, New X-Band and S-Band Linear Accelerators at Varex Imaging, LINAC2022, England, 2022.
- [12] Stanislav Proskin, Andrey Mishin, Devon Fischer, Maximizing Output of 3 MeV S-band Industrial Accelerator, IPAC2022, 2022.
- [13] M. Denney, R. LaFave, D. Fischer, J. Roylance, L. Young, S. Proskin, A. Mishin, High Power Test Results of Diode E-Gun Based 4-6 MeV Accelerator Beam Centerline (ABC), 7-12 May, Venezia, Italy, 2023.
- [14] J. Turner, L. Miller, D. Nichols, S. Wilson, P. Maeder, R. LaFave, M. Denney, J. Roylance, L. Young, D. Fischer, S. Proskin, A. Mishin, M3X Linac Subsystem for Security Screening, 18-24 June, Crete, Greece, 2023.
- [15] A. V. Mishin, New Accelerator Beam Centerline (ABC) Production Line at Varex Imaging Corporation, Proceedings of IPAC 2024, Nashville Tennessee, USA, 19-24 May 2024.
- [16] A. V. Mishin†, A. Amoroso, S. Proskin, J. Roylance, Rich LaFave, L. Miller, S. Wilson, New High Power Linear ABC and Platform, Proceedings of IPAC 2024, Nashville Tennessee, USA, 19-24 May 2024.
- [17] A. V. Mishin, High Energy Sources Development and Production at Varex Imaging Corporation, invited oral talk, CAARI 2024, Fort Worth, Texas, USA, 21-26 July 2024.
- [18] Andrey V. Mishin, Stanislav Proskin, Linear Accelerators with Submillimeter Beam Spot Size for Non-Destructive Testing and Security Screening, 20<sup>th</sup> World Conference on Non-Destructive Testing (20<sup>th</sup> WCNDT), Songdo Convensia, Incheon, Korea, May 2024.
- [19] A. Mishin, S. Proskin, R. LaFave, L. Miller, A. Amoroso, and J. Roylance, "New high power linear accelerator ABC and platform", presented at the IPAC'24, Nashville, TN, USA, May 2024, paper MOPC63.
- [20] A. V. Mishin, Accelerator structure for low-energy electron beam, Proceedings of International Conference on Particle Accelerators, 17-20 May 1993. <https://doi.org/10.1109/pac.1993.308713>
- [21] A. V. Mishin, Linear Accelerator for Low Power RF Sources, (extended and filed together with R. Schonberg, ref. 26). Patent Application, 1996.
- [22] A. V. Mishin, R. G. Schonberg, H. Deruyter, Microwave Power Control Apparatus for Linear Accelerator, Patent Application Serial No. 08/390,122, Docket No. OP/135, Filed February 17, 1995, Patent date August 26, 1997, US Patent 5,661,377.
- [23] A. V. Mishin, R. G. Schonberg CW Particle Accelerator with Low Particle Injection Velocity, Falk, Vestal & Fish, CA, USA, Patent Application Serial No. 08/764,535, Docket No. GEF-001, Filed December 12, 1996, Patent date April 28, 1998, US Patent 5,744,919.

- [24] A. V. Mishin, Status on low energy (10 MeV range) X-band linacs developed worldwide, Proceedings Particle Accelerator Conference, 01-05 May 1995.  
<https://doi.org/10.1109/pac.1995.504587>
- [25] H. Deruyter, A. V. Mishin, T. Roumbanis, R. G. Schonberg, R. Miller, J. Potter, Properties and Possible Applications of Multiple Beam Coupled Cavity Structure, Proceedings of EPAC-96, Barcelona, Spain, 1996.
- [26] H. Deruyter, A. V. Mishin, T. Roumbanis, R. G. Schonberg, S. Farrell, R. Smith, R. Miller, High Power 2 MeV Linear Accelerator Design Characteristics, Proceedings of EPAC-96, Barcelona, Spain, 1996.
- [27] A. V. Mishin, R. G. Schonberg, Portable Linear Electron Accelerators for Industrial Applications, Proceedings of 28th International SAMPE Technical Conference, Seattle, Washington, November 4-7, 1996.
- [28] A. V. Mishin, Portable linear electron accelerators for electron beam curing of composites, non-destructive testing and other applications, Structural Faults and Repair-97, 7<sup>th</sup> International Conference and Exhibition, Edinburg, Scotland, 8-10 July, 1997.
- [29] A. V. Mishin, R. G. Schonberg, H. Deruyter, T. Roumbanis, D. Skowbo, L. Begin, K. Voak, R. Wurster, E. Black, Schonberg Research Corporation, R. Miller, D. Yeremian, Y. Batygin, Portable Linac Using a CW Magnetron as a Power Source, Proc. of EPAC-98, Stockholm, Sweden, 1998.
- [30] A. V. Mishin, R. G. Schonberg, Hollow-beam Microwave Linear Accelerator, Patent Application Serial No. 08/717,859, Filed September 23, 1996, Patent date September 22, 1998, US Patent 5,811,943.
- [31] A. V. Mishin, Linear Accelerators for Non-Destructive Testing, ASNT-99, Rome, Italy, 1999.
- [32] H. Deruyter, R. Foote, A. V. Mishin, W. Sapp, R. G. Schonberg, D. Skowbo, Portable CW Linac for Commercial Applications, Proceedings of IPAC-99, New York, 1999.  
<https://doi.org/10.1109/pac.1999.795768>
- [33] R. D. Swift, W. Wade Sapp, A. V. Mishin, Relocatable Intermediate Energy X-ray Cargo Inspection Systems, 1999 ONDCP International Technology Symposium, 1999.
- [34] William Wade Sapp, Jr., Peter Rothschild, Richard Schueller, Andrey Mishin, New Low-dose 1 MeV Cargo Inspection System with Backscatter Imaging, The International Symposium on Optical Science and Technology, SPIE 45th Annual Meeting, San Diego, CA, 2000.  
<https://doi.org/10.1117/12.410560>
- [35] W. Wade Sapp, William L. Adams, Joseph Callera, Lee Grodzins, Peter J. Rothschild, Richard Schueller, Andrey V. Mishin, Relocatable X-Ray Cargo Inspection Systems utilizing Compact LINACs, AIP Conf. Proc. 576, 1057–1060 (2001), July 12, 2001. <https://doi.org/10.1063/1.1395487>
- [36] A. V. Mishin, “Advances in X-Band and S-Band Linear Accelerators for Security, NDT, and Other Applications”, in *Proc. PAC’05*, Knoxville, TN, USA, May 2005, paper FOAB002, p. 240. <https://doi.org/10.1109/pac.2005.1590405>
- [37] A. Saverskiy, H. Deruyter, M. Hernandez, A. V. Mishin, D. Skowbo, Portable X-Band Linear Electron Accelerators for Radiographic Applications, Proceedings of 2005 Particle Accelerator Conference, Knoxville, Tennessee, 2005.  
<https://doi.org/10.1109/pac.2005.1590981>
- [38] M. Hernandez, H. Deruyter; D. Skowbo, R. Smith, A. V. Mishin, A. Saverskiy, A 7MeV S-Band 2998MHz Variable Pulse Length Linear Accelerator System, Proceedings of 2005 Particle Accelerator Conference, Knoxville, Tennessee, 2005.  
<https://doi.org/10.1109/pac.2005.1590949>
- [39] A. V. Mishin, Pulse-to-Pulse-Switchable Multiple-Energy Linear Accelerators Based on Fast RF Power Switching, Filed: 8 March 2008, Patent US 2008/0211431, 4 September 2008.
- [40] A. V. Mishin, W. W. Sapp, P. Rothschild, Single-Pulse-Switched Multiple Energy X-Ray Source Applications, Patent Application Serial No. 11/931,431, Filed October 31, 2007, Patent date May 26, 2009, US Patent 7,538,325.
- [41] Richard True, The Design of Gridded Pierce Guns for Accelerators, IEEE Transactions on Nuclear Science, Volume 32, Issue 5, October 1985.  
<https://doi.org/10.1109/tns.1985.4333997>
- [42] R. True, Emittance and the Design of Beam Formation, Transport, and Collection Systems in Periodically Focused TWT’s, IEEE Transactions on Electron Devices, Vol. ED-34, No. 2, Part 2, February 1987.  
<https://doi.org/10.1109/t-ed.1987.22949>
- [43] V. A. Vaguine, Standing Wave High Gradient Accelerator Structure, Review of Scientific Instruments 48, 1658, 1977.  
<https://doi.org/10.1063/1.1134969>
- [44] J. Bigolas, S. Getka et al, The SW accelerating structure of variable energy electron linac for medical application, Proceedings of the 2001 Particle Accelerator Conference (Cat. No. 01CH37268). <https://doi.org/10.1109/pac.2001.987908>
- [45] VJ Technologies (for Varex Imaging Corporation, Internal Report), Varex M3 BCL Report, 2 March 2021.
- [46] Granpect Company Limited, Hextron, Marketing Brochure, [www.granpect.com](http://www.granpect.com) Beijing, China.
- [47] Norihito Matsunaga et al, Development of 950 kV X-ray source with small focal spot using a linear accelerator, 9th Conference on Industrial Computed Tomography, Padova, Italy (iCT 2019), <https://doi.org/10.58286/23647>
- [48] Norihito Matsunaga et al, Application of a compact X-ray source with small focal spot using a 950 keV linear accelerator, International Symposium on Industrial Radiology and Computed Tomography, DIR2019,  
<https://www.duerr-ndt.com/news/event/symposium-on-digital-industrial-radiology-and-computed-tomography-2019.html>
- [49] Norihito Matsunaga et al, CT performance of compact X-ray source with small focal spot using a 950 keV linear accelerator, 10th Conference on Industrial Computed Tomography, Wels, Austria (iCT 2020), <https://doi.org/10.58286/25095>

## Biography



**Andrey Valentinovich Mishin** is a Vice President, High Energy Systems (HES) at Varex Imaging Corporation, Headquartered in Salt Lake City, UT, USA. He graduated from National Research Nuclear University (MEPhI) in 1985 and completed his PhD equivalent in Charged Particle Accelerator Physics in 1992. Dr. Mishin has been in senior leadership positions with private and public companies in USA since 1995. He has completed Management of High-Technology Companies course with AeA Stanford Executive Institute in 2002. In 2024, Dr. Mishin was included in directory of top managers and professionals by Marquis Who's Who, "for his pioneering work in microwave devices and linear accelerators". Dr. Mishin is a member of the esteemed IEEE and of ASNT. Throughout

his 42-year career, he has spearheaded multiple major domestic and international projects, was an Invited Speaker, Session Co-Chair at international conferences. He was Chairman of a Sister City Committee with Santa Clara Government.

## Research Field

**Andrey Mishin:** Electron Beam Sources, X-Ray Sources, Linear Accelerators, Microwave Devices, Security Screening, Non-Destructive Testing, Electron Beam Processing, Radiation Oncology Systems, Intraoperative Radiation Oncology Systems